



Robert M. McMillan
"High Accuracy Measuring And Control Of Low
Fluid Flow Rate"
Albert B. Kimball,Jr. 713/221-1377
B&P Ref. 057723.000015
1/9




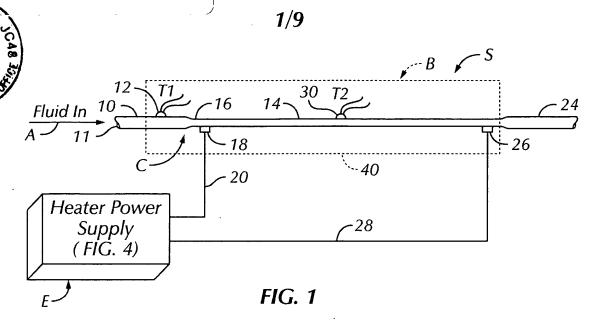

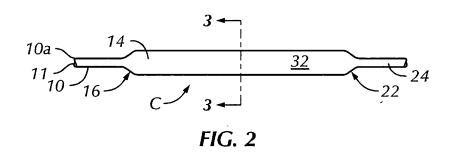



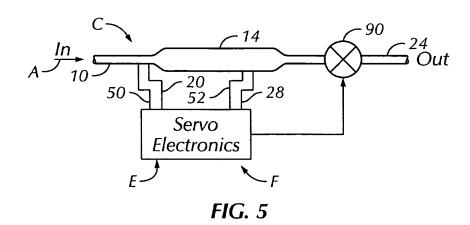

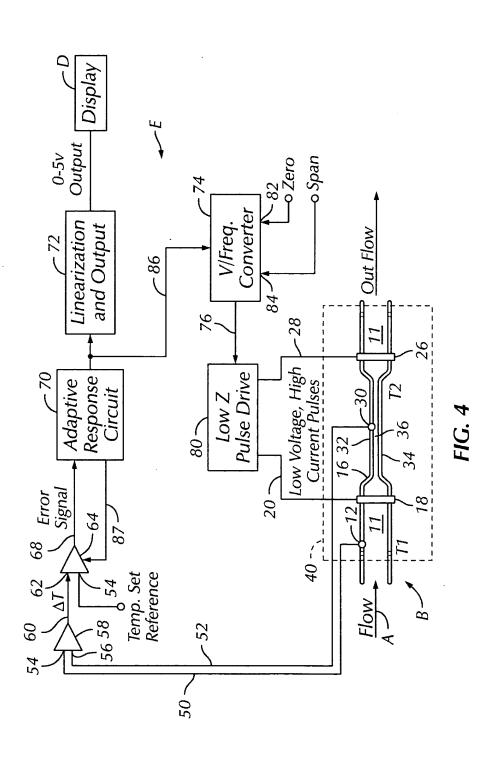

3/9

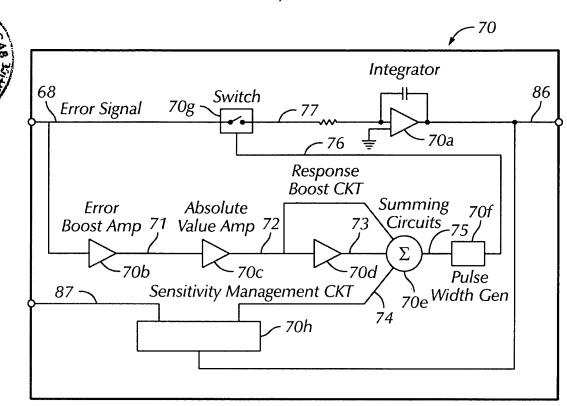


FIG. 6


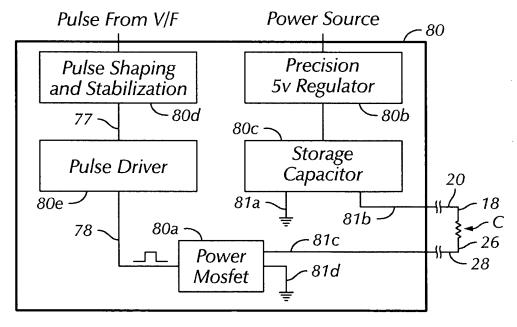


FIG. 7



/9

